



TEST REPORT TUCHENG

ORIGINAL

Date: Jun. 15, 2020 Date of Receipt: May. 28, 2020

Report No.: TFF9E618 Quantity: IPC Page Order/Pages: (P1/2) Ref. No.: NIL

Report Title: Aevoe Inc. (Moshi) (T7594) Item: Filter Media

Address: 27F., No. 8, Sec. 5, Zhongxiao E. Rd., Xinyi Dist., Taipei City 110, Taiwan

Test Items		Test Results	Test Methods
Bacterial Filtration	1	> 99.9	ASTM F2101-2019
Efficiency (BFE)(%)	2	> 99.9	
Staphylococcus aureus	3	> 99.9	
ATCC 6538	4	> 99.9	
	5	> 99.9	

Note: Control average: 1866 CFU.


Note: Mean particle size: 2.9 μ m.

Note: Testing side: outside of specimen.

Note: Testing area: 39.5 cm².

Note: Flow rate : 28.3 L/min.

Note: Sample description is given by the client: Nanohedron TM filters

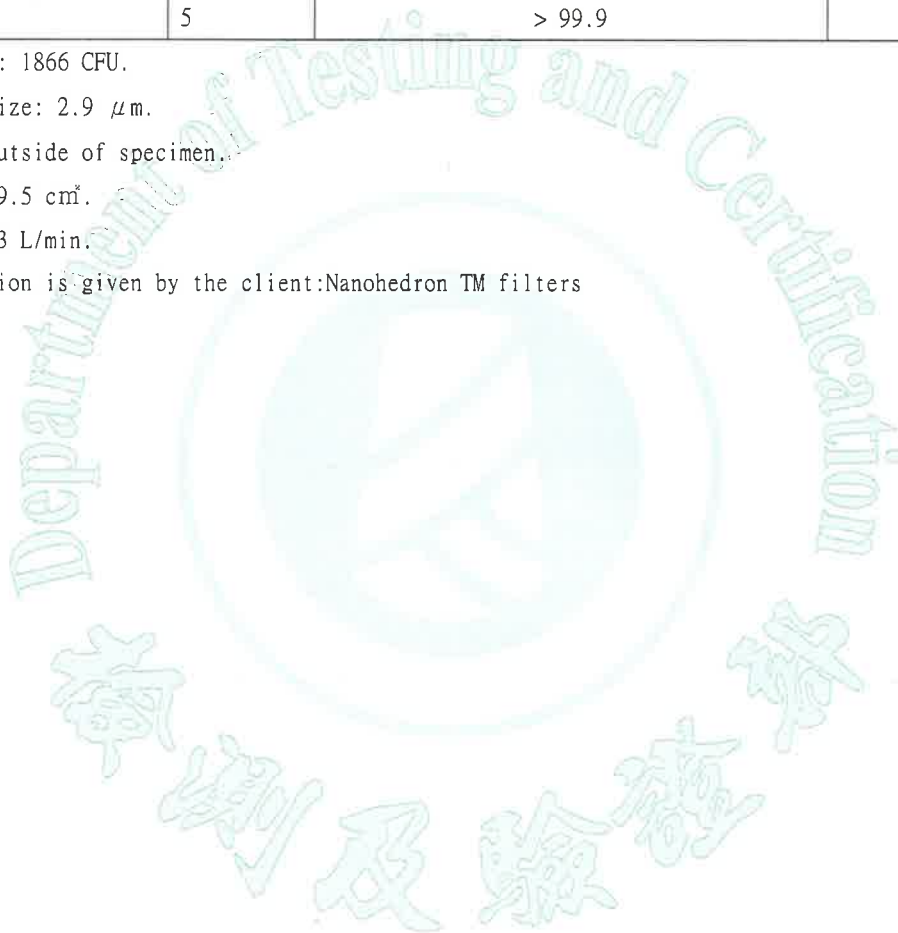

Note: 1. This report is only responsible for the submitted sample(s), which will be kept for one month period.

2. This report cannot be reproduced in any way, except in full context, without the prior approval in writing of this Department of Testing and Certification.

3. The test report should not be used for public advertisement and commercial promotion.

Authorized by president of
Taiwan Textile Research Institute

Jui-hung Kao

Director,
Department of Testing and Certification

Department of Testing and Certification, Taiwan Textile Research Institute
No.6, Chengtian Rd., Tucheng Dist., New Taipei City 23674, Taiwan (R.O.C.)
Tel : +886-2-22670321 ext. 7107, 7110
Fax : +886-2-22675108, +886-2-22689839



TEST REPORT TUCHENG

ORIGINAL

Date: Jun. 15, 2020 Date of Receipt: May. 28, 2020

Report No.: TFF9E618 Quantity: 1PC Page Order/Pages: (P2/2) Ref. No.: NIL

Report Title: Aevoe Inc. (Moshi) (T7594) Item: Filter Media

Address: 27F., No. 8, Sec. 5, Zhongxiao E. Rd., Xinyi Dist., Taipei City 110, Taiwan



- Note: 1. This report is only responsible for the submitted sample(s), which will be kept for one month period.
2. This report cannot be reproduced in any way, except in full context, without the prior approval in writing of this Department of Testing and Certification.
3. The test report should not be used for public advertisement and commercial promotion.

Authorized by president of
Taiwan Textile Research Institute

Jui-hung Kao

Director,
Department of Testing and Certification
Taiwan Textile Research Institute
No. 6, Chengtian Rd., Tucheng Dist., New Taipei City 23674, Taiwan (R.O.C.)
Tel : +886-2-22670321 ext. 7107, 7110
Fax : +886-2-22675108 , +886-2-22689839